




Morse Spreaders

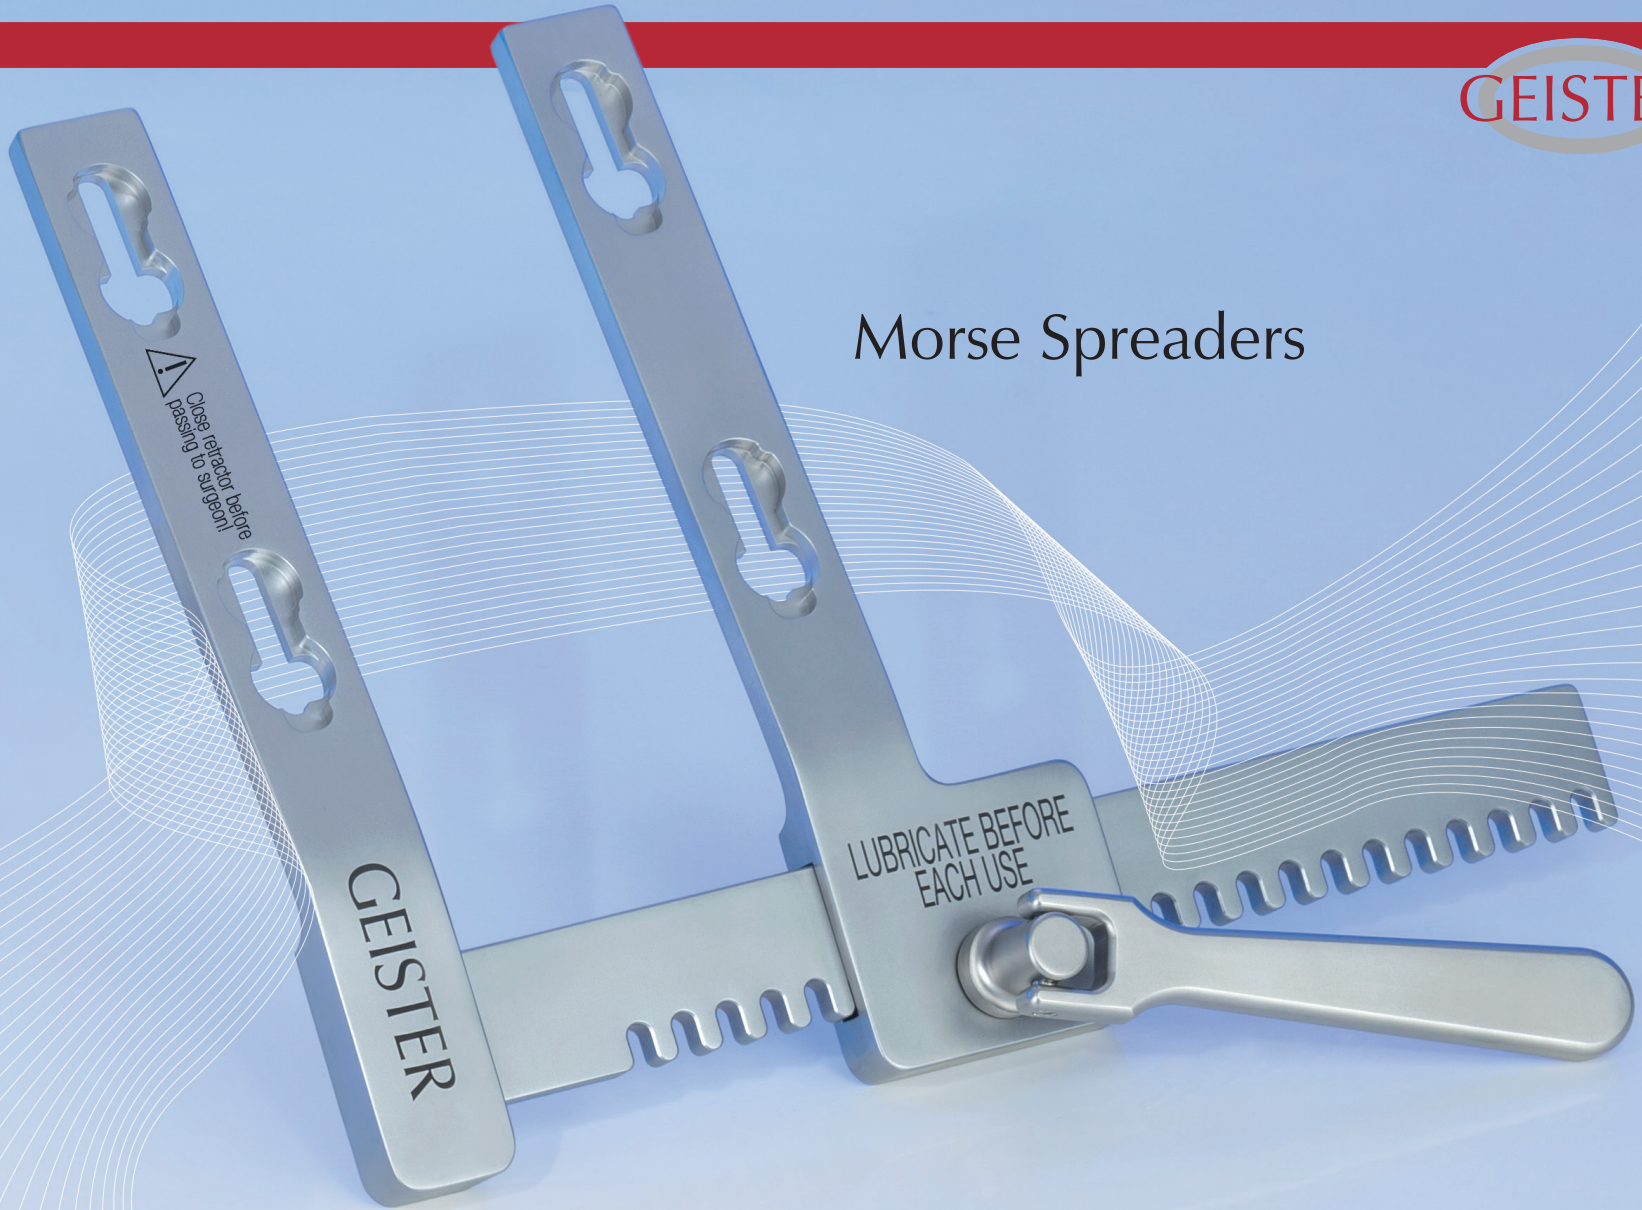

Close retractor before passing to surgeon!

GEISTER

LUBRICATE BEFORE EACH USE